




Die Kalibrier-Profis



# Beta Master Cal 990

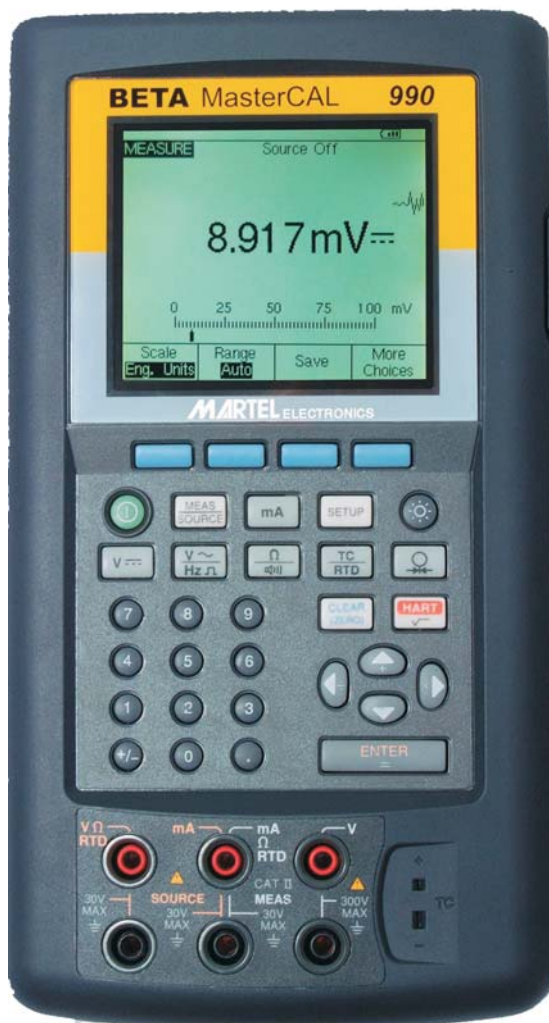

#### Eigenschaften:

- präziser Multifunktionskalibrator mit HART Schnittstellenkommunikation in einem Gerät
- Messen von Thermoelementen, Widerstandsthermometern, Widerständen, DC und AC Spannungen DC Strömen, Druck und Frequenz
- Simulieren/Geben von Thermoelementen, Widerstandsthermometer, Widerständen, DC Spannung und Strom, Druck und Frequenz.
- paralleles Messen und Geben durch geteiltes Display möglich
- Stromschleifen Funktionen
- Transmitter Modus
- Automatische und benutzerdefinierte Funktionen
- Standardeinheiten, Prozentskalen, Wurzelfunktionen und benutzerdefinierte Einheiten
- mehrsprachiges Menü (Englisch, Französisch, Deutsch, Italienisch und Spanisch)
- 200 x 240 Pixel LCD Display mit Hintergrundbeleuchtung
- sehr robustes Urethan Gehäuse für den Vor Ort-Einsatz
- Automatische Kalibrierung und Dokumentation mit den meisten dem Markt befindlichen Softwarepaketen möglich

# Multi-Function Documenting Calibrator

## MasterCAL 990

### General Features

- Precision multi-function calibrator and HART™ configurator/communicator in one hand-held instrument
- Measure/read thermocouple, RTD, Ohms, DC and AC Voltage, DC current, pressure, and frequency
- Source/simulate thermocouple, RTD, Ohms, DC Voltage and current, pressure, and frequency
- Simultaneous input and output split-screen displays
- Loop power function
- Switch testing functions
- Transmitter mode
- Automated and user-programmable procedures
- Engineering units, percent of scale, squarelaw inputs, or custom units
- Multi-lingual interface – English, French, German, Italian, and Spanish
- 200x240 pixel, bright white, backlit LCD display
- Rugged over-molded urethane case for field use
- Calibration automation and documentation with many popular third-party software packages
- Complies with CAN/CSA C22.2 No 1010.1-92, ANSI/ISA S82.01-1994, UL3111, and

### HART Protocol Features

- Universal, common practice and devicespecific Commands
- Point-to-point and multi-drop operation
- Burst mode compatibility
- Read HART PV in digital mode
- Read and write HART configuration functions
- Read and clone transmitter configuration
- Re-tag smart transmitters
- Automated HART sensor and output trim

### The MasterCAL 990 - A Precision Multi-Function Documenting Calibrator

First and foremost, the MasterCAL 990 is a precision, multi-function documenting calibrator that will calibrate virtually any process instrument you have – thermocouples, RTDs, Ohms, Voltage, current, pressure, and frequency. A host of convenience features, including source ramp functions, loop power, variable density data logging with a week's worth of calibration results storage, compatibility with many third-party calibration documentation software programs, and a built-in HART configuration/communicator, make the MasterCAL 990 an indispensable tool.

A large, white backlit LCD provides simultaneous display of input and output. Menu-driven, "soft" function keys provide rapid setup and measurement. The multilingual interface ensures the MasterCAL 990 is useful in as broad a range of applications and locations as possible. A high capacity rechargeable battery pack provides extended usage. An optional battery eliminator is available for extended monitoring applications. The MasterCAL 990 is housed in an over-molded urethane case that provides a solid grip and protection against "hard knocks".

### Source/Simulation

The MasterCAL 990 will source/simulate thermocouple, RTD, Ohms, DC Voltage and current, and frequency. Auto-step and ramp functions are provided on all outputs and Ranges.

### Measurement/Read

The MasterCAL 990 will measure/read thermocouple, RTD, Ohms, DC and AC Voltage, DC current, pressure, and frequency. Measuring pressure requires the use of the Beta Pressure Module Adapter (Model BPPA100) with any of Beta's Pressure Modules (please refer to the separate Pressure Module data sheet for ranges and Accuracies).

# Multi-Function Documenting Calibrator MasterCAL 990

## Switch Test Mode

Process limit switches can be tested for both upper and lower trip limits and deadband. Using a split-screen measure/source mode, the MasterCAL 990 accepts a normal process variable measurement associated with the limit switch, and the switch contacts. The 990 will automatically monitor and record the measurement as the switch is activated and then deactivated. A graphical plot of deadband is displayed, making switch test quick and accurate.

## Simultaneous Measure/Source

Using a split-screen display mode, the MasterCAL 990 will simultaneously measure and source various process variables. These variables depend on whether loop power is enabled or disabled. Please refer to Table 1.

## Transmitter Mode

The MasterCAL 990 can be inserted in a 4-20 mA process loop to simulate a 2-wire transmitter. The MasterCAL 990 provides the loop excitation and modulates the loop current, simulating the 2-wire transmitter.

## Built-In Calculator Functions

The MasterCAL 990 features a built-in calculator with square-root function, with accessible registers containing measure and source values.

## Barcode Entry Option

The MasterCAL 990 will accept input from an optional barcode wand for rapid entry of instrument serial numbers.

**Table 1 – Simultaneous Measure/Source**

Measure Function	Source Function					
	DC V	mA	Freq	$\Omega$	TC	RTD
DC V	DE	D	DE	DE	DE	DE
mA	DE		DE	DE	DE	DE
AC V	DE	D	DE	DE	DE	DE
Frequency ( $\geq 20$ Hz)	DE	D	DE	DE	DE	DE
Frequency ( $< 20$ Hz)						
$\Omega$	D		D	D	D	D
Continuity	D		D	D	D	D
TC	DE	D	DE	DE		DE
RTD	D		D	D	D	D
3W RTD	D		D	D	D	D
4W RTD	D		D	D	D	D
Pressure	DE	D	DE	DE	DE	DE

Simultaneous measure/source works with:  
D= Loop power disabled; E= Loop power enabled

# Multi-Function Documenting Calibrator

## MasterCAL 990

### HART Implementation

The MasterCAL 990 supports HART Version 5.7 protocol instructions. Its functions are comparable to a HART 275 Communicator; because the MasterCAL 990 does not have a DD interpreter, it does not support DD libraries. Most instrument maintenance functions can be accomplished using just the MasterCAL 990 without the need for a separate HART communicator. Hookup is simple with the supplied HART interface cable. The calibrator menus automatically branch to appropriate adjustment choices. Automatic completion of test templates and automatic fetching and sending of analog readings during trim operations make HART calibration a highly efficient operation.

### Protocol Instructions

The MasterCAL 990 instruction set includes three levels of commands:

**Universal Commands** – provides functions for all field instruments to read manufacturer and device type, primary variable/input signal (PV), read output, tag ID, etc.

**Common Practice Commands** – provides functions that are common to most field instruments, such as reading multiple variables, setting damping features, etc.

**Device-Specific Commands** – allows the MasterCAL 990 to perform device-specific configuration functions for a wide variety of popular field instruments. Please refer to Table 2.


### Operating Modes

The MasterCAL 990 supports HART Point-to-Point Operation, where a single HART instrument is connected in a loop; the calibrator is normally connected directly at the instrument's local signal terminals. The MasterCAL 990 is also compatible with multi-drop and burst mode HART Installations.

### Documenting Calibration

The MasterCAL 990 is compatible with many third-party calibration documentation software programs including:

- Applied Systems Technologies Cal Station and Base Station
- Emerson Process Management AMS
- Prime Technologies ProCal
- Fluke DPC Track
- Honeywell DocuMint
- Others supporting the ISA Field Calibrator Interface standard

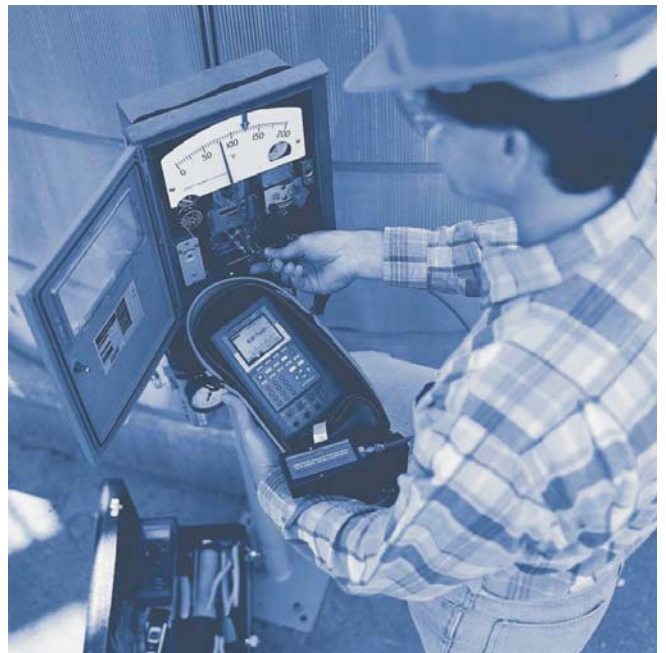

# Multi-Function Documenting Calibrator MasterCAL 990

## Manufacturer

ABB/Kent-Taylor  
ABB/Hartmann & Braun  
Endress & Hauser

Foxboro Eckardt  
Foxboro/Invensys

Honeywell  
Moore Products  
Rosemount

Siemens

SMAR  
Viatran  
Wika  
Yokogawa

## Pressure Instruments

600T  
Contrans P 1, AS 800 Series  
CERABAR S,  
CERABAR M,

I/A Pressure

St3000  
344 1  
1151  
2088  
3001C  
3051, 3051S  
SITRANS P DS  
SITRANS P ES  
Ld301  
I/A Pressure  
UNITRANS  
EJA

## Temperature Instruments

658T 1  
TMT 122 1, TMT 182 1,  
TMT 162 1  
T1/RTT20 1

STT25T 1, STT25H 1

3044C  
644  
3144  
3244, 3144P

TT301 1

T32H 1  
YTA 110, 310, and 320

*1 Sensor Trim not supported*



# Multi-Function Documenting Calibrator

## MasterCAL 990

### Specifications (18 °C to 28 °C unless otherwise noted)

#### DC Voltage Read and Source

Measurement Range/Accuracy (% of reading + % of full scale; 1 year; 2 year)	
0.000 to 110.000 mV	±0.025% rdg. +0.015%FS
0.000 to 1.10000 V	±0.05% rdg. +0.015%FS ±0.025% rdg. +0.005%FS
0.000 to 11.0000 V	±0.05% rdg. +0.005%FS ±0.025% rdg. +0.005%FS
0.000 to 110.000 V	±0.05% rdg. +0.005%FS ±0.025% rdg. +0.005%FS
0.000 to 300.00 V	±0.1% rdg. +0.005%FS ±0.05% rdg. +0.005%F ±0.1% rdg. +0.005%FS
Read Input Impedance	5 Mohms
Read Common Mode Error	±0.008% FS/V
Read Input Voltage	300 V rms maximum
Temperature Coefficient	(±0.001% rdg + -10 °C to 18 °C, and 28°C to 50 °C

#### AC Voltage Read (10% to 100% of range)

Measurement Range/Accuracy (% of reading + counts; 1 year; 2 year)	
20 to 40 Hz	±2% rdg. +10 ±2% rdg. +10
40 to 500 Hz	±0.5% rdg. +5 ±0.5% rdg. +5
500 Hz to 1 kHz	±2% rdg. +10 ±2% rdg. +10
1 to 5 kHz	±10% rdg. +20 ±10% rdg. +20
Read Input Voltage	
Minimum Ranges	0.5 V above 1 kHz 1.1000 V, 11.000 V, 110.00 V, 300.0 V
Maximum	300 V rms
Read Input Impedance	5 MOhms and <100 pF
Read Input Coupling	AC only
Read Common Mode Error	±0.008% FS/V
Temperature Coefficient	±10% of spec/°C; -10 °C to 18 °C, and 28°C to 50 °C

#### Source Range/Accuracy

(% of reading + % of full scale; 1 year; 2 year)	
0.000 to 110.000 mV	±0.01% rdg. +0.005%FS ±0.015% rdg. +0.005%FS
0.000 to 1.10000 V	±0.01% rdg. +0.005%FS ±0.015% rdg. +0.005%FS
0.000 to 15.0000 V	±0.01% rdg. +0.005%FS ±0.015% rdg. +0.005%FS
Source Output Loading	(±0.001% FS + 1 µV)/mA
Source Common Mode Error	0.008% FS/V
Source Output Current	10 mA maximum
Source Output Voltage	30 VDC maximum
Temperature Coefficient	(±0.001% rdg + 0.001% FS)/°C; -10 °C to 18 °C, and 28 °C to 50 °C

#### DC Current Read and Source

Measurement Range/Accuracy (% of output + % of full scale; 1 year; 2 year)	
0.000 to 30.000 mA	±0.01% +0.015%FS ±0.02% +0.015%FS
0.000 to 110.000 mA	±0.01% +0.015%FS ±0.02% +0.015%FS
Read Common Mode Error	±0.01% FS/V
Read Input Voltage	30 VDC maximum
Temperature Coefficient	(±0.001% rdg + 0.002% FS)/°C; -10 °C to 18 °C, and 28°C to 50 °C
Source Range/Accuracy (% of output + % of full scale; 1 year; 2 year)	
0.000 to 22.000 mA	±0.01% +0.015%FS ±0.02% +0.015%FS
Transmitter simulate (current sink)	±0.02% rdg. +0.005%FS ±0.015% rdg. +0.005%FS
Source Burden Voltage	24 V maximum
Source Common Mode Error	0.008% FS/V
Source Input Voltage	30 VDC maximum
Temperature Coefficient	(±0.003% output + 0.003% FS)/°C; -10 °C to 18 °C, and 28°C to 50 °C

# Multi-Function Documenting Calibrator

## MasterCAL 990

### Ohms Read and Source

Measurement Range/Accuracy  
(% of reading + Ohms; 1 year; 2 year)

0.000 to 11.000 Ohms	±0.05% + 50 m. ±0.075% + 50 m.
0.000 to 110.00 Ohms	±0.05% + 50 m. ±0.075% + 50 m.
0.000 to 1.1000 kOhms	±0.05% + 0.5 . ±0.075% + 0.5 .
0.000 to 11.000 kOhms	±0.1% + 10 . ±0.1% + 10 .

Read Common Mode Error	±0.005% FS/V
Read Input Voltage	30 VDC maximum
Continuity	continuous tone <<25 .; no tone >400 .
Temperature Coefficient	(±0.01% FS + 2 m.)°C; -10 °C to 18 °C, and 28°C to 50 °C

Source Range/Accuracy  
(% of output + Ohms; 1 year; 2 year)

0.000 to 11.000 Ohms	±0.01% + 20 m. ±0.02% + 20 m.
0.000 to 110.00 Ohms	±0.01% + 40 m. ±0.02% + 40 m.
0.000 to 1.1000 kOhms	±0.02% + 0.5 . ±0.03% + 0.5 .
0.000 to 11.000 kOhms	±0.03% + 5 . ±0.04% + 5 .
Read Common Mode Error	±0.008% FS/V
Source Input Voltage	30 VDC maximum
Current Through Source Resistance	
11.000 Ohms range	3 mA DC max.; 0.1 mA DC min.
11.000 Ohms range	3 mA DC max.; 0.1 mA DC min.
11.000 Ohms range	3 mA DC max.; 0.01 mA DC min.
11.000 Ohms range	1 mA DC max.; 0.01 mA DC min.
Temperature Coefficient	±0.01% FS/°C; -10 °C to 18 °C, and 28 °C to 50 °C

### Frequency Read and Source

(For frequencies <109.99 Hz, specification applies for signals with slew rates >5 V/ms)

Measurement Range/Accuracy (1 year; 2 year)	
1.00 to 109.99 Hz	±0.05 Hz ±0.05 Hz
110.0 to 1099.9 Hz	±0.5 Hz ±0.5 Hz
1.100 to 10.999 kHz	±0.005 Hz ±0.005 Hz
11.00 to 50.00 kHz	±0.05 kHz ±0.05 kHz

Minimum Input Amplitudes	
1 Hz to 1 kHz squarewave	300 mVP-P
1 kHz to 30 kHz squarewave	1.4 VP-P
>30 kHz	
Maximum Input Amplitudes	
1 Hz to 1 kHz	300 V rms
>1 kHz	30 V rms
Input Impedance	5 Mohms

Source Range/Accuracy  
(1 year; 2 year)

0.00 to 10.99 Hz	±0.01 Hz ±0.01 Hz
11.00 to 109.99 Hz	±0.1 Hz ±0.1 Hz
110.0 to 1099.9 Hz	±0.1 Hz ±0.1 Hz
1.100 to 21.999 kHz	±0.002 kHz ±0.002 kHz
22.00 to 50.00 kHz	±0.005 kHz ±0.005 kHz
Waveforms	squarewave with 50% duty cycle sinewave
Amplitude	0.1 to 10 VP-P; User-adjustable
Amplitude Accuracy	
1 to 1099 Hz	±3% of output + 0.5% FS
1.1 to 10.9 kHz	±10% of output + 0.5% FS
11 to 50 kHz	±30% of output + 0.5% FS
Input Voltage	30 VDC maximum

# Multi-Function Documenting Calibrator

## MasterCAL 990

### Thermocouple Read and Source

(Accuracies with external cold junction; add 0.2 °C for internal junction; sensor inaccuracies not included)

Resolution	0.1 °C
Temperature Scale	ITS-90 or IPTS-68, selectable
Compensation	ITS-90 per Monograph 175 for E/N/J/K/T/B/R/S thermocouples IPTS-68 per IEC 584-1 for E/J/K/T/B/R/S thermocouples  IPTS-68 per DIN 43710 for L and U Thermocouples
Input Voltage	30 VDC maximum
Common Mode Error	0.01 °C/V
Temperature Coefficient	0.05 °C/°C; -10 °C to 18 °C, and 28 °C to 50 °C

### Read Type/Range/Accuracy (1 year; 2 year)

#### J Thermocouple year)

-210 to -100 °C	±0.6 °C; ±0.9 °C
-100 to +800 °C	±0.3 °C; ±0.4 °C
+800 to +1200 °C	±0.5 °C; ±0.8 °C

#### K Thermocouple

-210 to -100 °C	±0.7 °C; ±1.0 °C
-100 to +400 °C	±0.3 °C; ±0.4 °C
+400 to +1200 °C	±0.5 °C; ±0.8 °C
+1200 to +1372 °C	±0.7 °C; ±1.0 °C

#### T Thermocouple

-250 to -200 °C	±1.7 °C; ±2.5 °C
-200 to 0 °C	±0.6 °C; ±0.9 °C
0 to +400 °C	±0.3 °C; ±0.4 °C

#### E Thermocouple

-250 to -200 °C	±1.3 °C; ±2.0 °C
-200 to -100 °C	±0.5 °C; ±0.8 °C
-100 to +600 °C	±0.3 °C; ±0.4 °C
+600 to +1000 °C	±0.4 °C; ±0.6 °C

#### R Thermocouple

-20 to 0 °C	±2.3 °C; ±2.8 °C
0 to +100 °C	±1.5 °C; ±2.2 °C
+100 to +1767 °C	±1.0 °C; ±1.5 °C
+100 to +1767 °C	±1.0 °C; ±1.5 °C

#### S Thermocouple

-20 to 0 °C	±2.3 °C; ±2.8 °C
0 to +200 °C	±1.5 °C; ±2.1 °C
+200 to +1400 °C	±0.9 °C; ±1.4 °C
+1400 to +1767 °C	±1.1 °C; ±1.7 °C

#### B Thermocouple

+600 to +800 °C	±1.3 °C; ±2.0 °C
+800 to +1000 °C	±1.0 °C; ±1.5 °C
+1000 to +1820 °C	±0.9 °C; ±1.3 °C

#### B Thermocouple

+600 to +800 °C	±1.0 °C; ±1.5 °C
+800 to +1000 °C	±0.8 °C; ±1.2 °C
+1000 to +1820 °C	±0.8 °C; ±1.2 °C

#### C Thermocouple

0 to +800 °C	±0.6 °C; ±0.9 °C
+800 to +1200 °C	±0.7 °C; ±1.0 °C
+1200 to +1800 °C	±0.9 °C; ±1.4 °C
+1800 to +2316 °C	±1.3 °C; ±2.0 °C

#### L Thermocouple

-200 to -100 °C	±0.3 °C; ±0.4 °C
-100 to +800 °C	±0.2 °C; ±0.3 °C
+800 to +900 °C	±0.2 °C; ±0.3 °C

#### C Thermocouple

0 to +800 °C	±0.6 °C; ±0.9 °C
+800 to +1200 °C	±0.8 °C; ±1.2 °C
+1200 to +1800 °C	±1.1 °C; ±1.6 °C
+1800 to +2316 °C	±2.0 °C; ±3.0 °C

#### L Thermocouple

-200 to -100 °C	±0.6 °C; ±0.9 °C
-100 to +800 °C	±0.3 °C; ±0.4 °C
+800 to +900 °C	±0.5 °C; ±0.8 °C

#### U Thermocouple

-200 to 0 °C	±0.6 °C; ±0.9 °C
0 to +600 °C	±0.3 °C; ±0.4 °C

#### N Thermocouple

-200 to -100 °C	±1.0 °C; ±1.5 °C
-100 to +900 °C	±0.5 °C; ±0.8 °C
+900 to +1300 °C	±0.6 °C; ±0.9 °C

### Source Type/Range/Accuracy (1 year; 2

#### J Thermocouple

-210 to -100 °C	±0.3 °C; ±0.4 °C
-100 to +800 °C	±0.2 °C; ±0.3 °C
+800 to +1200 °C	±0.2 °C; ±0.3 °C

#### K Thermocouple

-210 to -100 °C	±0.4 °C; ±0.6 °C
-100 to +400 °C	±0.3 °C; ±0.4 °C
+400 to +1200 °C	±0.3 °C; ±0.4 °C
+1200 to +1372 °C	±0.3 °C; ±0.4 °C

#### T Thermocouple

-250 to -200 °C	±0.9 °C; ±1.4 °C
-200 to 0 °C	±0.4 °C; ±0.9 °C
0 to +400 °C	±0.3 °C; ±0.4 °C

#### E Thermocouple

-250 to -200 °C	±0.6 °C; ±0.9 °C
-200 to -100 °C	±0.3 °C; ±0.4 °C
-100 to +600 °C	±0.3 °C; ±0.4 °C
+600 to +1000 °C	±0.2 °C; ±0.3 °C

#### R Thermocouple

-20 to 0 °C	±1.2 °C; ±1.8 °C
0 to +100 °C	±1.1 °C; ±1.7 °C
0 to +100 °C	±1.1 °C; ±1.7 °C
+100 to +1767 °C	±0.9 °C; ±1.4 °C

#### S Thermocouple

-20 to 0 °C	±1.2 °C; ±1.8 °C
0 to +200 °C	±1.1 °C; ±1.7 °C
+200 to +1400 °C	±0.9 °C; ±1.4 °C
+1400 to +1767 °C	±1.0 °C; ±1.5 °C

#### U Thermocouple

-200 to 0 °C	±0.4 °C; ±0.6 °C
0 to +600 °C	±0.3 °C; ±0.4 °C

#### N Thermocouple

-200 to -100 °C	±0.6 °C; ±0.9 °C
-100 to +900 °C	±0.5 °C; ±0.8 °C
+900 to +1300 °C	±0.3 °C; ±0.4 °C

Note: When simulating temperature in As Found/As Left procedures, steps may be either linear by temperature or linear by mV potential.

# Multi-Function Documenting Calibrator MasterCAL 990

## RTD Read and Source

(For 2-wire or 3-wire measurements, add 0.4 °C;  
-sensor inaccuracies not included)  
Resolution 0.1 °C, except 1 °C for  
10 . Cu  
Input Voltage 30 VDC maximum  
Input Current for RTD Source Function  
10, 100, 120 Ω RTDs 8 mA DC  
200, 500, 1000 Ω RTDs 1 mA DC  
addresses pulsed  
transmitters and PLCs  
with pulses as short  
as 1 ms  
Temperature Coefficient 0.02 °C/°C;  
-10 °C to 18 °C, and 28°C  
to 50 °C

### Read Type/Range/Accuracy (1 year; 2 year)

Cu10	
-100 to 0 °C	±2.0 °C; ±2.0 °C
0 to +260 °C	±2.0 °C; ±2.0 °C
Pt100 (3916)	
-200 to -190 °C	±0.3 °C; ±0.4 °C
-190 to 0 °C	±0.3 °C; ±0.4 °C
0 to +630 °C	±0.5 °C; ±0.8 °C
Pt100 (3926)	
-200 to 0 °C	±0.3 °C; ±0.4 °C
0 to +630 °C	±0.5 °C; ±0.8 °C
Pt100 (385)	
-200 to 0 °C	±0.3 °C; ±0.5 °C
0 to +400 °C	±0.5 °C; ±0.8 °C
+400 to +800 °C	±0.8 °C; ±1.0 °C
Pt200 (385)	
-200 to 0 °C	±0.3 °C; ±0.5 °C
0 to +400 °C	±0.5 °C; ±0.8 °C
+400 to +630 °C	±0.8 °C; ±1.0 °C
Pt500 (385)	
-200 to 0 °C	±0.3 °C; ±0.5 °C
0 to +400 °C	±0.5 °C; ±0.8 °C
+400 to +630 °C	±0.8 °C; ±1.0 °C
Pt1000 (385)	
-200 to 0 °C	±0.3 °C; ±0.5 °C
0 to +400 °C	±0.5 °C; ±0.8 °C
+400 to +630 °C	±0.8 °C; ±1.0 °C
Ni120 (672)	
-80 to +260 °C	±0.3 °C; ±0.4 °C
Source Type/Range/Accuracy (1 year; 2 year)	
Cu10	
-100 to 0 °C	±1.0 °C; ±1.0 °C
0 to +260 °C	±1.0 °C; ±1.0 °C

Pt100 (3916)	
-200 to -190 °C	±0.3 °C; ±0.4 °C
190 to 0 °C	±0.1 °C; ±0.2 °C
0 to +630 °C	±0.2 °C; ±0.4 °C
Pt100 (3926)	
-200 to 0 °C	±0.1 °C; ±0.2 °C
0 to +630 °C	±0.2 °C; ±0.4 °C
Pt100 (385)	
-200 to 0 °C	±0.1 °C; ±0.2 °C
0 to +400 °C	±0.2 °C; ±0.4 °C
+400 to +800 °C	±0.4 °C; ±0.5 °C
Pt200 (385)	
-200 to 0 °C	±0.1 °C; ±0.2 °C
0 to +400 °C	±0.2 °C; ±0.4 °C
+400 to +630 °C	±0.4 °C; ±0.5 °C
Pt500 (385)	
-200 to 0 °C	±0.1 °C; ±0.2 °C
0 to +400 °C	±0.2 °C; ±0.4 °C
+400 to +630 °C	±0.4 °C; ±0.5 °C
Pt1000 (385)	
-200 to 0 °C	±0.1 °C; ±0.2 °C
0 to +400 °C	±0.2 °C; ±0.4 °C
+400 to +630 °C	±0.4 °C; ±0.5 °C
Ni120 (672)	
-80 to +260 °C	±0.1 °C; ±0.2 °C

## Pressure Read and Source

Please refer to the Beta Pressure Module Data Sheet, 030606R0 for ranges and accuracies. Requires use of included BPPA100 Pressure Module Adapter.



# Multi-Function Documenting Calibrator MasterCAL 990

## General

### Loop Power

Voltage	24 V or 28 V, selectable
Maximum Current:	22 mA, short-circuit protected
Input Voltage	30 VDC maximum
Accuracy	5%

Note: A 250Ω series resistance is automatically supplied whenever loop power is enabled.

### Ramp Functions

Source Functions	Voltage, current, Ohms, frequency, temperature
Rate	4 steps/second
Trip Detect	continuity or voltage; continuity detection not available when sourcing current

### Data Log Function

Measure Functions	Voltage, current, Ohms, frequency, temperature, pressure
Reading Rate	1, 2, 5, 10, 20, 30, or 60 readings/minute
Maximum Record Length	8,000 readings 7,980 for 30 or 60 readings/minute

### Environmental

Operating Temperature	-20 °C to +50 °C -10 °C to +50 °C for in spec frequency and AC read
Storage Temperature	-20 °C to +60 °C
Altitude	9,186 ft (2800 m) above mean sea level
Stability (90 day)	Typical 90-day measurement/read and source/simulate accuracy can be estimated by dividing the one year “% of reading” or “% of output” specifications by 2. Floor specifications, expressed as “% of FS” or “counts” or “Ohms” remain constant

### Power Requirements

Battery	7.2 VDC NiMH rechargeable, 3500 mAh; included
Battery Life	>8 hours, typical usage

### Physical

Dimensions	9.3"H x 5.1"W x 2.4"D (236 x 130 x 61 mm)
Weight	3 lbs, 1 oz. (1.4 kg)
Connectors/Ports	Pressure module connector RS232 serial

### Included Accessories

External power in  
Test lead set (4 leads, test clips, test probes)  
NimMH battery pack  
Battery pack charger  
Deluxe carrying case  
BPPA100 Pressure Module Adapter  
Serial port cable  
HART communications cable  
NIST-traceable calibration certificate, with data  
Multi-lingual instruction manual on CD  
Warranty registration card

### Optional Accessories

Barcode wand



**Klasmeier Kalibrier- und Messtechnik GmbH**

Browerstraße 39, D-36039 Fulda - Germany

Tel.: +49 (0) 661 55011 Fax: +49 (0) 661 57498

E-Mail: [info@klasmeier.com](mailto:info@klasmeier.com) Internet: [www.klasmeier.com](http://www.klasmeier.com)